


# HT7800 Transmission Electron Microscope Instruction

Startup procedure:

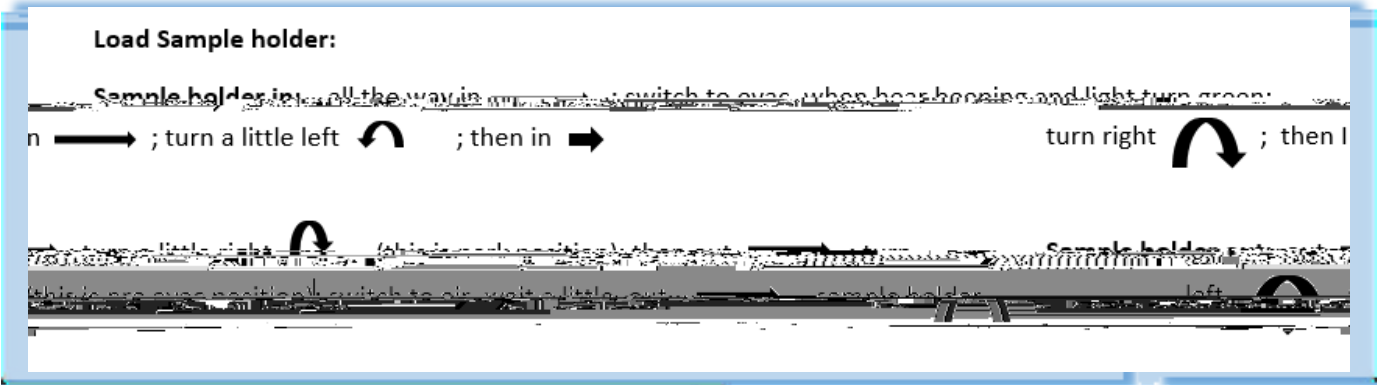

“on”


“on”

“Zoom-1”, “HC-1”,

“BH”.

Hitachi TEM system control  
(main window)

Transmission image

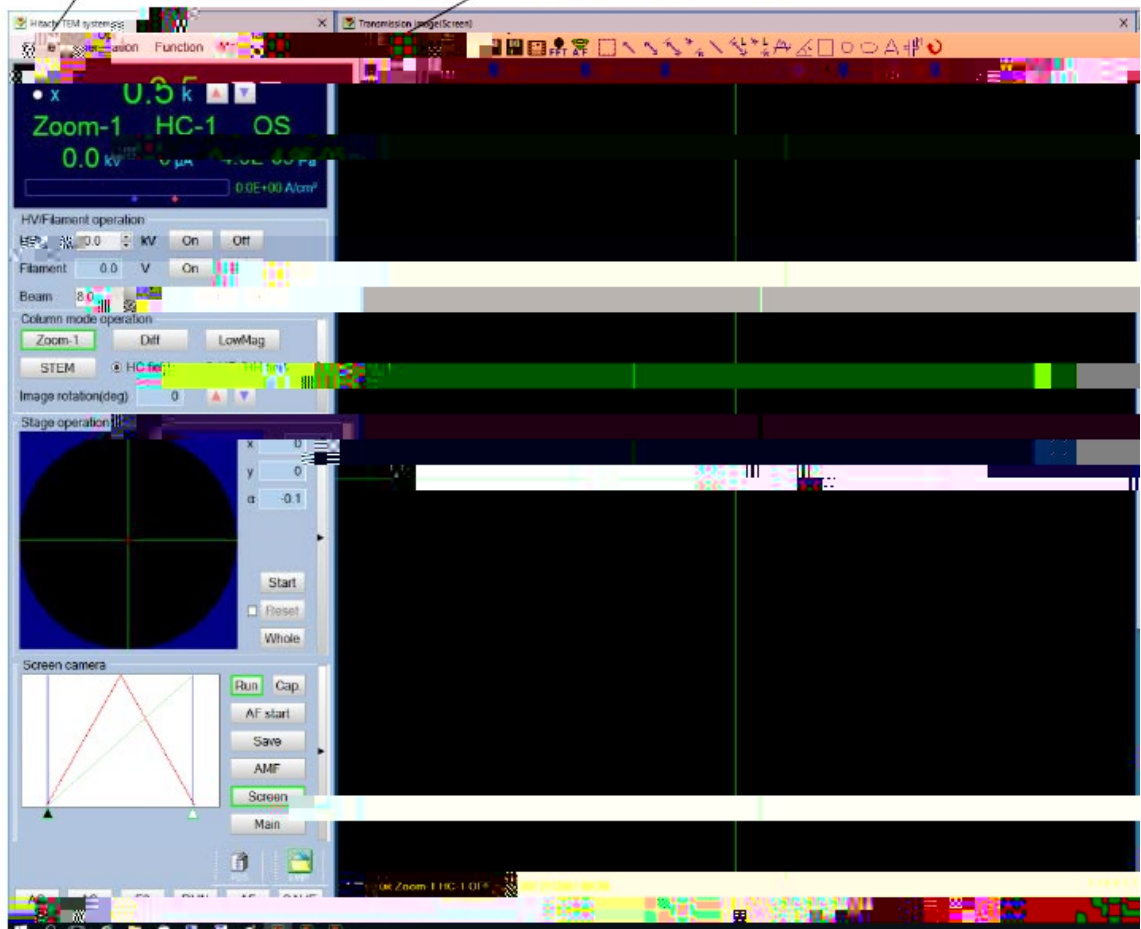

Screen”

“auto LUT”

R

Holder tab  
holder reset”

“lens”

Centering the beam:

knob

Put in the Objective aperture

aperture:

X and Y knob

brightness

Adjusting the objective

**Change magnification and move sample position:**

**Magnification knob**

**tracker ball**

**Focus image:**

**“AF start”**

**focus knob**

**Adjusting**